



Strap-On Pipe Radiation Monitor

Model Series PEMO-7 PEMO-7, PEMO-7-MCA, PEMO-7-G

Features

- Installs Anytime Anywhere
- Sensitivity Independent of Flow Rate
- No Penetration, No Downtime
- Sensitivity: 1×10^{-7} $\mu\text{Ci/cc}$ ^{60}Co in 18" Pipe
- Real Time Alarm
- Rate and Integrated Exposure
- Detector Type Choice: NaI (TI) or HPGe
- USB and Ethernet Ports
- On Board Data Archive, Transmit, and Display

Application

The **PEMO-7** Pipe Monitor assures accurate detection and quick alarm in case of waterborne radioactivity contamination flowing thru one or more pipes. A constant check with alarm and data record is accomplished by the onboard computer. Integrated exposure information is recorded and can provide a hard copy

via external printer. It is a complete system and may be expanded per need with modules of the FM-9 series. The **PEMO-7** is sensitive and versatile. It may be used to monitor water in pipes or effluent streams down to EPA levels.

Description

The **PEMO-7** uses standard NaI (TI) Detector in T/A's unique Strap-On Style Shield to continuously measure any water or airborne gamma emitting Radioactive contaminants, onboard data logging. The water or air stream is under constant surveillance via a scintillation detector. The unit is completely self-contained.

- **PEMO-7** utilizes a NaI (TI) scintillation crystal detector.
- **PEMO-7-MCA** utilizes a NaI (TI) scintillation crystal detector.
- **PEMO-7-G** utilizes an intrinsic HPGe solid state detector.

Note for Selection of *Intrinsic HPGe* Detector, PEMO-7-G

The **PEMO-7-G** System has an installed Dewar to maintain HPGe crystal at proper temperature range.


Optional: An electronic cryo-cooler is available.



TECHNICAL ASSOCIATES OVERHOFF TECHNOLOGY


7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303
PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@USNUCLEARCORP.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM


DIVISIONS OF
 USNUCLEARCORP
OTCQB-UCLE

Strap-On Pipe Radiation Monitor

Model Series PEMO-7
PEMO-7, PEMO-7-MCA, PEMO-7-G

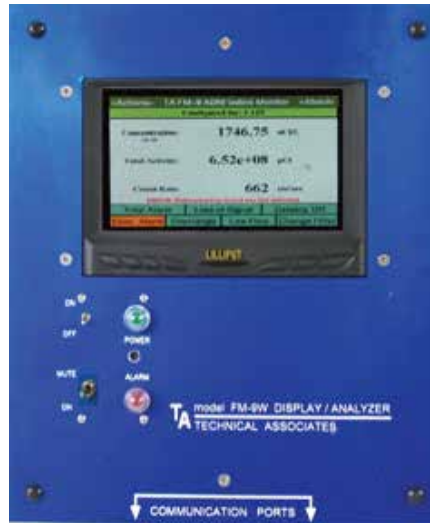


ELECTRONICS
Model FM-9W

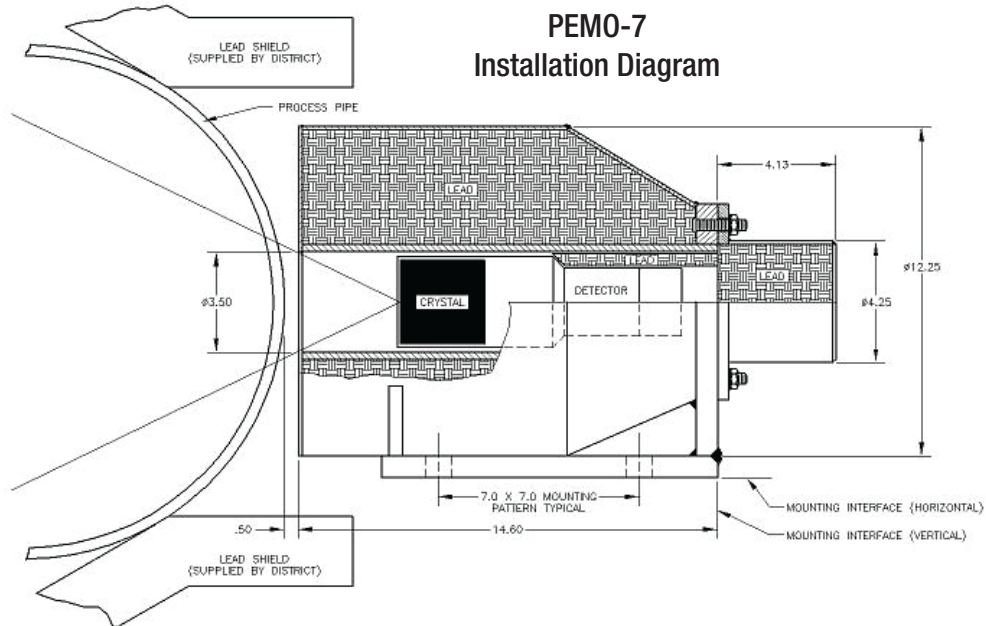

**TECHNICAL ASSOCIATES
OVERHOFF TECHNOLOGY**

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303
PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@USNUCLEARCORP.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISIONS OF
 USNUCLEARCORP
OTCQB-UCLF

Strap-On Pipe Radiation Monitor

Model Series PEMO-7 PEMO-7, PEMO-7-MCA, PEMO-7-G

Specifications

Sensitivity

Sensitivity and response time depend on user's requirements and physical circumstances such as pipe diameter, wall thickness, and ambient background radiation level and energy (KeV) of major nuclides of interest.

Example: The standard system with 3" x 3" NaI detector and 2" of lead shielding has a limit of sensitivity better than 1×10^{-7} Ci/cc of ^{60}Co in an 18" diameter pipe with 0.02 mR/hr background in a one hour measurement.

Detectors

PEMO-7 and PEMO-7-MCA 3" x 3" NaI (TI) crystal scintillation detector probe
Model PGS-3 x 3T (typically one per pipe) with sensitivity to all Gamma above 100 KeV

PEMO-7-G Intrinsic HPGe Solid State Detector

Electronics

Engineering Units: User can input correct conversion factor and change to any units

Controls: Front Panel: On-Off, Alarm-Mute, Rate, Integrate, Reset

Recessed or Internal: Discriminator level, High voltage, other adjustable settings: See calibration

Input Sensitivity: Adjustable from less than 1 millivolt to 100 millivolt
Anti-saturation and Dead-time corrections are available

Alarm: 2000 Hz audio tone with audio "mute" switch + RED LIGHT
High current relay. 0-100% of full scale

Alarm Set Point: User settable to any point on detector range

Serial Output: Two way USB standard, Ethernet optional

Power: 105-125 volts, 50-60 Hz (220 V optional)

- **Optional:** Software package for integration into facility computer and to link multiple detectors

Electronics Dimensions and Weight

21" W x 11" H x 16" D
20 pounds (9 kg)

MODEL	ENERGY ANALYZER	DETECTOR	SMART ELECTRONICS	ANALYSIS OUTPUT	TEMPERATURE OPERATION
PEMO-7	Single Channel Analyzer (SCA)	3" x 3" NaI (TI)	FM-9W	Wide or Narrow Window	No Dewar Ambient Temperature Operation
PEMO-7-MCA	Multi-Channel Analyzer (MCA)	3" x 3" NaI (TI)	Full Computer	Isotope Identification Enhanced Display	No Dewar Ambient Temperature Operation
PEMO-7-G	Multi-Channel Analyzer (MCA)	HPGe Solid State	Full Computer	Isotope Identification Enhanced Display	Manual Dewar or Electronic Cryo-Cooler Cryogenic Temperature Operation



TECHNICAL ASSOCIATES OVERHOFF TECHNOLOGY

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303
PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@USNUCLEARCORP.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISIONS OF



USNUCLEARCORP

OTCQB-UCLF

Strap-On Pipe Radiation Monitor

Model Series PEMO-7 PEMO-7, PEMO-7-MCA, PEMO-7-G

Shielding:	0.25" to 3" low- activity-lead around detector.
Range: PEMO-7	Example: 1×10^{-7} to 1×10^{-4} $\mu\text{Ci/cc}$ with 3" x 3" NaI (TI) and 18" Pipe.
Alarm:	User Settable. 2000 Hz beeper, red flasher and relay contacts for user.
Response Time:	Settable from 1 second to 10 minutes.
Readout:	Color Monitor showing: concentration, total activity and programmed information.
Power:	115 V, 50-60 Hz (230 V optional).
Flow Rate:	Measurement is independent of Flow rate.
Sample Volume:	The pipe should be full of liquid for best sensitivity.
Case:	Electronics rack mounted or housed in enameled steel case.

Weight and Dimensions

Detector Assembly Weight:	10 lbs for unshielded PEMO-7 assembly, up to 350 lbs for 2" thick lead shielding.
Shipping Weight:	450 lbs. for complete 1 detector PEMO-7 system, including detector light shielding. (weight will vary dependent on shield and detector selection)

Notes for Radiation Measurement When Detector is Outside of The Pipe Obstacles in Obtaining Good Efficiency and High Sensitivity When Measuring Radioactive Activity from the Outside of a Pipe.

1. Unknown volume if pipe is not always full
2. Unknown list of nuclides and energies
3. Pipe wall thickness and material, such as steel will absorb all Alphas and all Betas below 1 MeV, and Gammas below 100 KeV
4. Geometry of measurement is poor because pipe presents only a small angle source to the probe crystal's view

Units of Measurement for Pipe Monitor

Instrument can calculate and display any engineering units desired. But the user needs to input a valid calibration coefficient factor.

In the absence of a good calibration factor for the **PEMO-7**, read-out defaults to units in cps or can easily be set to read-out in **cpm** without calibration. Units of **mR/hr** can be set with minimum effort.

Instructions for Manual Input of Calibration Coefficient

1. Fill the pipe full with a known concentration of the single nuclide of greatest interest or abundance
2. Set energy window or area of interest to the major energy peak
3. Record the count rate



TECHNICAL ASSOCIATES OVERHOFF TECHNOLOGY

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303
PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@USNUCLEARCORP.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISIONS OF



USNUCLEARCORP

OTCQB-UCLE

Strap-On Pipe Radiation Monitor

Model Series PEMO-7 PEMO-7, PEMO-7-MCA, PEMO-7-G

4. Calculate calibration coefficient factor.


Calculation Formula:

Divide cps by Bq (Counts per second divided by disintegrations per second).

- Repeat procedure for the second most abundant nuclide.
- Use the factors that you have determined to calculate a weighted average factor which reflects the abundance of each important nuclide in the liquid mixture.
- Input the calibration factor as you follow the on-screen calibration instructions.
- The **PEMO-7** can then readout in concentration units such as $\mu\text{Ci/L}$ (microCuries per liter) or KBq/m^3 or as desired.

Note: Solid sources can be used to approximate the correct calibration factor for particular nuclides if pipe thickness is taken into account.

Optional Software Screen Shots

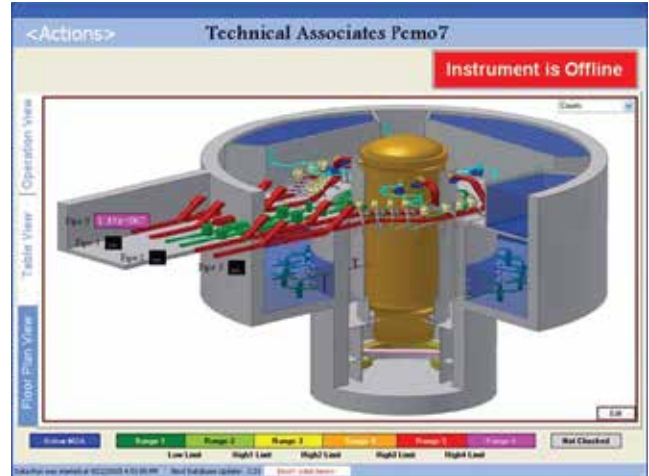

Location:	Pipe 0	Pipe 1	Pipe 2	Pipe 3
Status:	OK	Offline	Offline	Offline
Total Counts:	1.45e+007	---	---	---
Counts Per Second:	611	---	---	---
Dose Rate:	611 mR/h	---	---	---
Dose:	1.45e+007 mR	---	---	---


Measurable Name	EUs	Units	Counts Per Second	EUs (2 min Average)	EUs (30 min Average)	EUs (8 hr Average)	EUs (24 hr Average)	Limit Level	Loss Of Signal
Pipe 0 Counts		counts							<input type="checkbox"/>
Pipe 0 Count Rate		cps							<input type="checkbox"/>
Pipe 0 Dose Rate		mR/h							<input type="checkbox"/>
Pipe 0 Dose		mR							<input type="checkbox"/>
Pipe 1 Counts		counts							<input type="checkbox"/>
Pipe 1 Count Rate		cps							<input type="checkbox"/>
Pipe 1 Dose Rate		mR/h							<input type="checkbox"/>
Pipe 1 Dose		mR							<input type="checkbox"/>
Pipe 2 Counts		counts							<input type="checkbox"/>
Pipe 2 Count Rate		cps							<input type="checkbox"/>
Pipe 2 Dose Rate		mR/h							<input type="checkbox"/>
Pipe 2 Dose		mR							<input type="checkbox"/>
Pipe 3 Counts		counts							<input type="checkbox"/>
Pipe 3 Count Rate		cps							<input type="checkbox"/>
Pipe 3 Dose Rate		mR/h							<input type="checkbox"/>
Pipe 3 Dose		mR							<input type="checkbox"/>



TECHNICAL ASSOCIATES OVERHOFF TECHNOLOGY

7051 ETON AVENUE, CANOGA PARK, CALIFORNIA 91303
PHONE: 818-883-7043 | FAX: 818-883-6103

SALES@USNUCLEARCORP.COM | TECH-ASSOCIATES.COM | USNUCLEARCORP.COM

DIVISIONS OF
 USNUCLEARCORP
OTCQB-UCLC